

## GFP-Trap® capture surface for Biacore assays

GFP-Trap is a specific and stable binding molecule for green fluorescent protein (GFP)-tagged proteins convenient for usage in a Biacore capture assay format. GFP-Trap also recognizes proteins tagged with enhanced GFP (eGFP) and yellow fluorescent protein derivatives (YFP, eYFP and Venus).

This capture system allows an easy and effective isolation and

directed immobilization of fluorescent fusion proteins from complex biological samples like prokaryotic or eukaryotic cell extracts. Immobilization of these proteins enables binding studies and kinetic analysis using Biacore systems. With the GFP-Trap capture system valid data on localization, dynamics and mobility of proteins can be directly combined with interaction analysis using Biacore systems.




### Protocol

This protocol describes mainly how to immobilize and regenerate GFP-Trap.

#### 1. Immobilization of the GFP-Trap to an immobilization level around ~3000 RU

- Dilute GFP-Trap to 50 µg/ml in 10 mM acetate pH 5.5
- Coupling chemistry: Amine coupling
- Activation time: 7 min, ligand contact time: 7 min, deactivation time: 7 min
- Flow rate: 10 µl/min
- Sensor Chip CM5
- Immobilize the GFP-Trap on both the active and reference surface

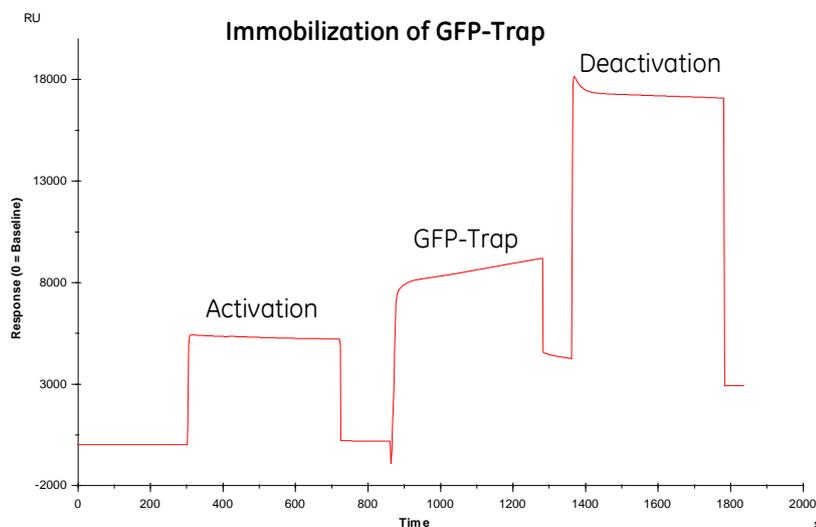

## 2. Capture of a GFP-tagged protein

You can calculate how much ligand you need on the sensor surface to give a desired theoretical  $R_{max}$  (maximum binding capacity for analyte) using the following formula:

$$R_{max} = \frac{\text{Analyte } M_w}{\text{Ligand } M_w} \times R_L \times S_m$$

$R_{max}$  [RU] = Maximal binding response

$R_L$  [RU] = Immobilization level

$S_m$  = Stoichiometric ratio

$M_w$  [Da] = Molecular weight

For kinetic analysis use low immobilization levels, typically a theoretical  $R_{max}$  value between 50-100 RU. In practice, the experimental  $R_{max}$  is usually somewhat lower than the theoretical value.

## 3. Investigate binding of your analyte to the GFP-tagged protein

- Start with a pM dilution of the GFP-tagged protein.
- If the concentration of the GFP-tagged protein in the extract is not known, set up a number of 10-times dilutions in running buffer. Start testing with the lowest concentration.
- Inject the analyte over both the active (GFP-tagged protein captured to GFP-Trap) and reference surface (GFP-Trap).

## 4. Regenerate the GFP-tagged protein from the GFP-Trap surface

- Use Glycine pH 2.0
- Contact time: 45 s
- Flow rate: 30  $\mu$ l/min

For local office contact information, visit  
[www.gelifesciences.com/contact](http://www.gelifesciences.com/contact)

[www.gelifesciences.com/biacore](http://www.gelifesciences.com/biacore)

GE Healthcare Bio-Sciences AB  
Björkgatan 30  
751 84 Uppsala  
Sweden

GE, imagination at work and GE monogram are trademarks of General Electric Company.  
Biacore is a trademark of GE Healthcare companies.

GFP-Trap is a trademark of ChromaTek and available at [www.chromotek.com](http://www.chromotek.com)

© 2011 General Electric Company—All rights reserved.

First published June 2011

All goods and services are sold subject to the terms and conditions of sale of the company within GE Healthcare which supplies them. A copy of these terms and conditions is available on request. Contact your local GE Healthcare representative for the most current information.

GE Healthcare UK Ltd  
Amersham Place, Little Chalfont, Buckinghamshire, HP7 9NA  
UK

GE Healthcare Bio-Sciences Corp  
800 Centennial Avenue, P.O. Box 1327, Piscataway, NJ 08855-1327  
USA

GE Healthcare Europe GmbH  
Munzinger Strasse 5, D-79111 Freiburg,  
Germany

GE Healthcare Japan Corporation  
Sanken Bldg. 3-25-1, Hyakunincho, Shinjuku-ku, Tokyo 169-0073  
Japan

28-9855-93 AB 08/2011